


Model 8800P

Orders should include the part number, model number, and instrument serial number. Call Teledyne Analytical Instruments at +1-888-789-8168 (USA Only) or +1-626-934-1500 to place an order for spare parts. Contact your regional sales representative for instrumentation questions; see <http://ai.www-uat.teledyne.com/en-us/who-we-are/worldwide-representatives>.

* These are internal parts and Teledyne does not recommend replacement in the field. The spare desiccant chamber has Viton washers included.

Replacement parts:

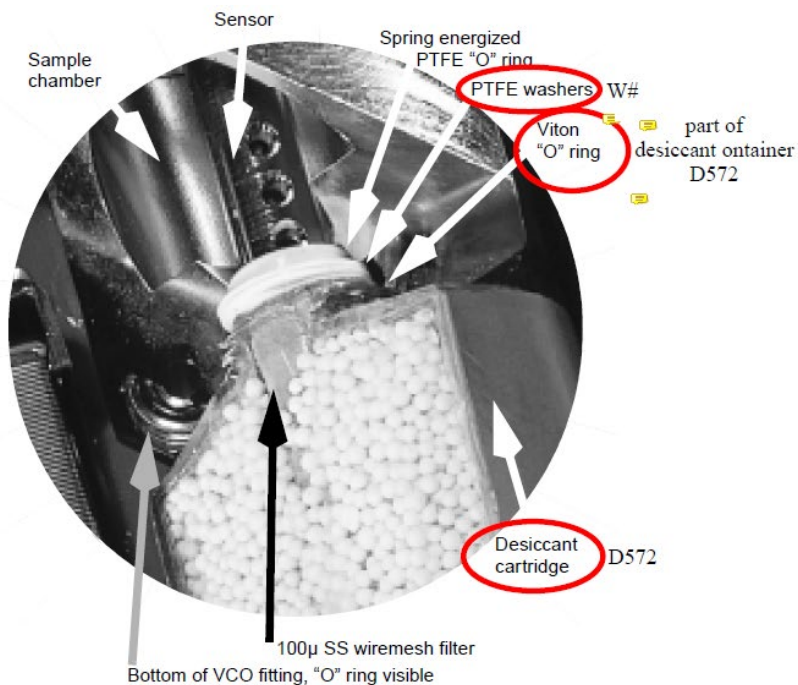

Bottom view of 8800P with cover open. The sample chamber and desiccant cartridge are shown cut open to facilitate an understanding of the mechanism and how it is assembled.



TELEDYNE
ANALYTICAL INSTRUMENTS
Everywhere you look™

16830 Chestnut Street, City of Industry, CA 91748 USA
Phone: 626-934-1500/888-789-8168 Fax: 626-934-1651
EMAIL: Ask_tai@teledyne.com www.teledyne-ai.com

Find your local sales representative: <http://ai.www-uat.teledyne.com/en-us/who-we-are/worldwide-representatives>